SUPERVISOR TEST

WASHINGTON COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 106406

Date: 06/17/2019

OPERATOR NAME:
KYLE L KOLAR
Permit #: 44063
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:33
INTERNAL STANDARD	VERIFIED	15:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:35
BLANK TEST	0.00	15:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:36
BLANK TEST	0.00	15:37
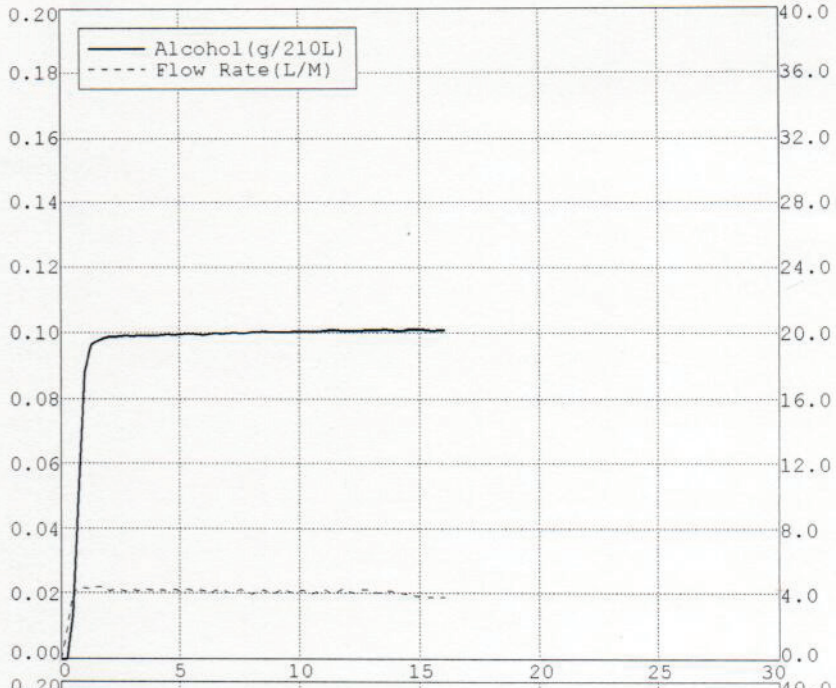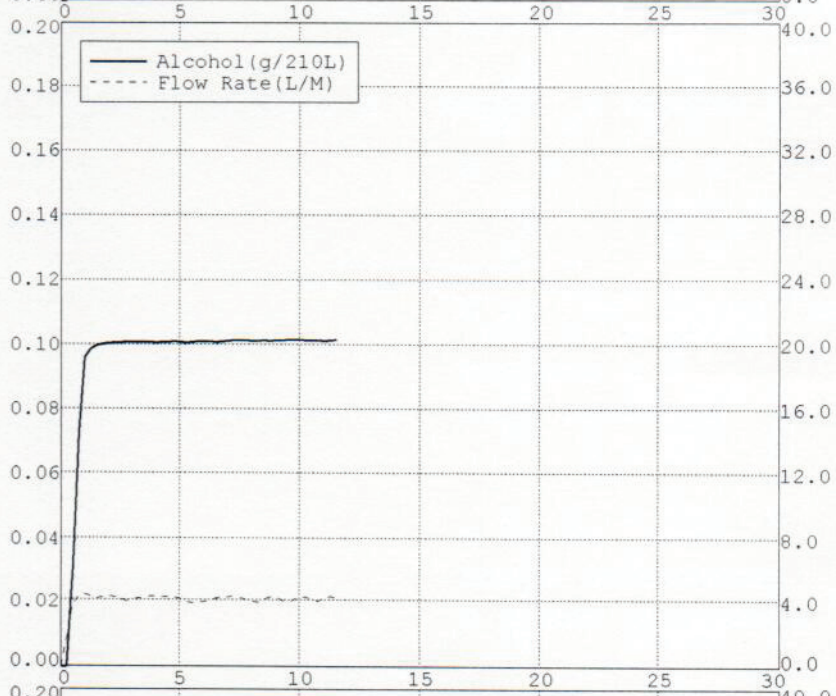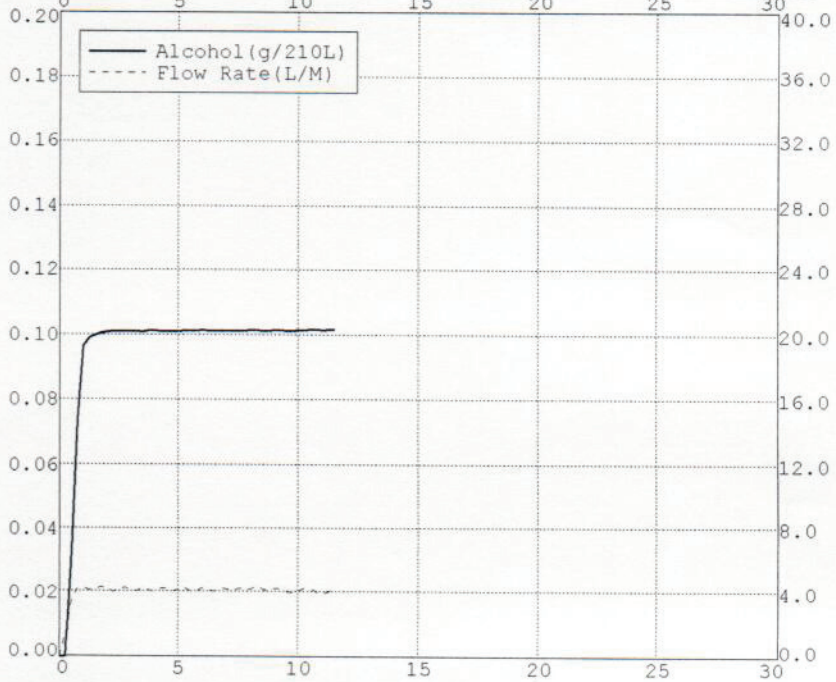
#691