

SUPERVISOR TEST




WASHINGTON CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 100284

Date: 04/08/2019

OPERATOR NAME:
MATTHEW K JACKSON
Permit #: 40078
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:34
INTERNAL STANDARD	VERIFIED	13:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:35
BLANK TEST	0.00	13:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:36
BLANK TEST	0.00	13:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:37
BLANK TEST	0.00	13:38

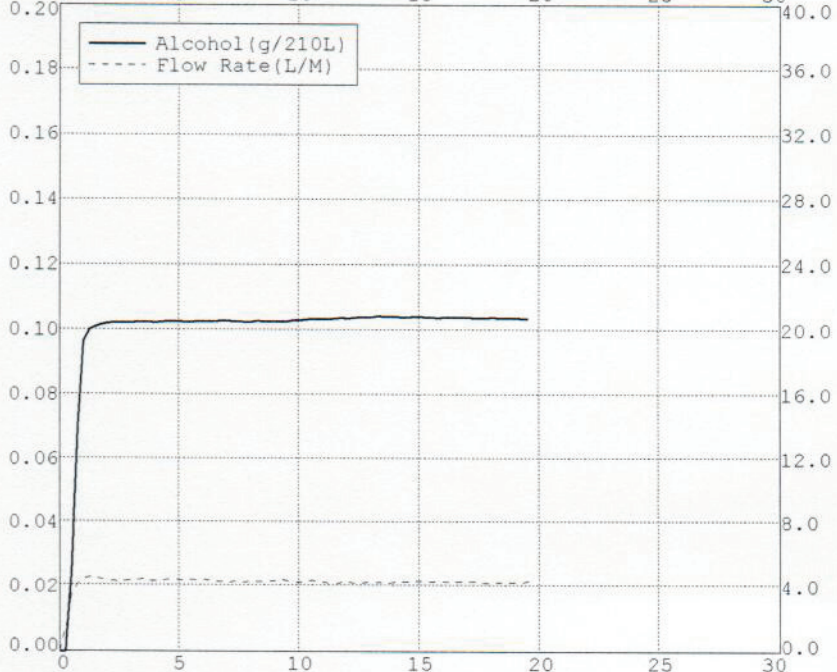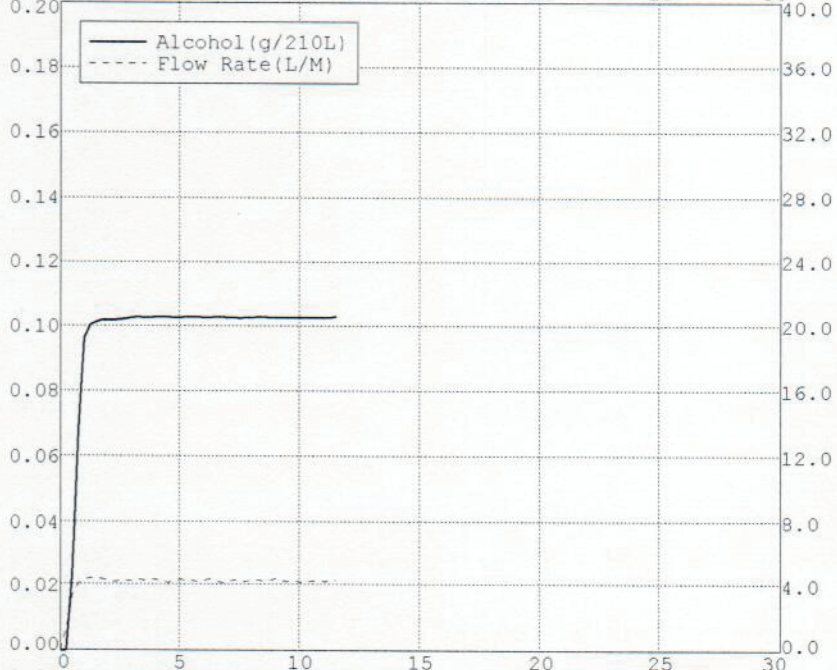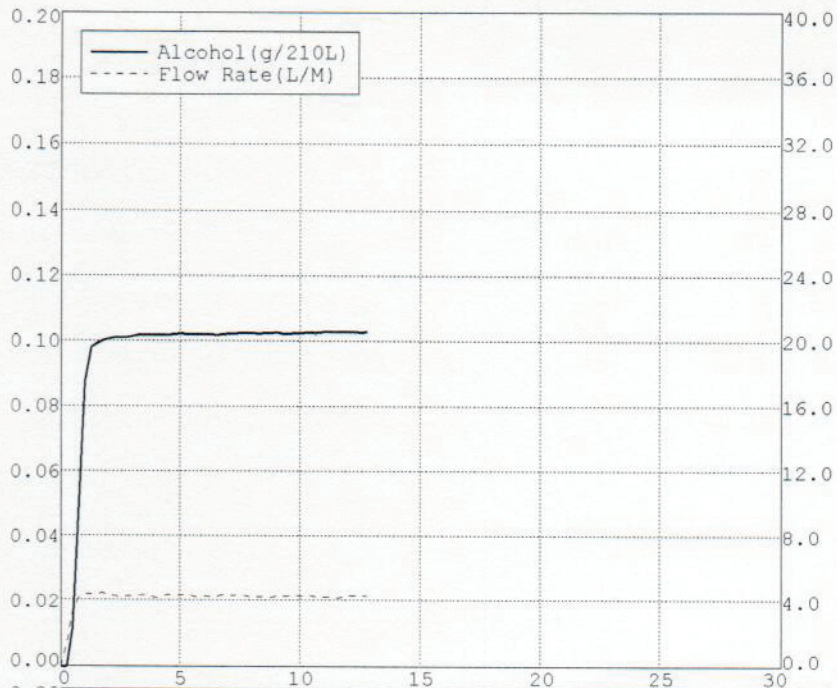

MAT #693