01-15-2020

To: Kristan Roth

From: Chief Ernie B.

Weekly Datamaster Test for GPD

7 pages

SUPERVISOR TEST

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

)ate: 01/11/2020

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:08
INTERNAL STANDARD	VERIFIED	22:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:08
BLANK TEST	0.00	22:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:09
BLANK TEST	0.00	22:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:11
BLANK TEST	0.00	22:11

SUPERVISOR TEST

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

Date: 12/28/2019

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:44
INTERNAL STANDARD	VERIFIED	21:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:44
BLANK TEST	0.00	21:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:46
BLANK TEST	0.00	21:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:47
BLANK TEST	0.00	21:47

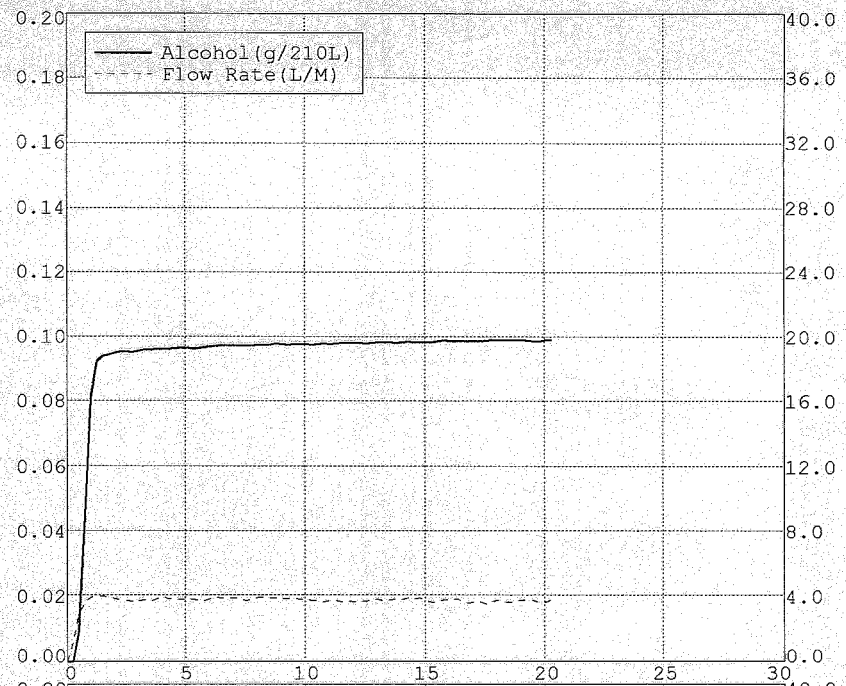

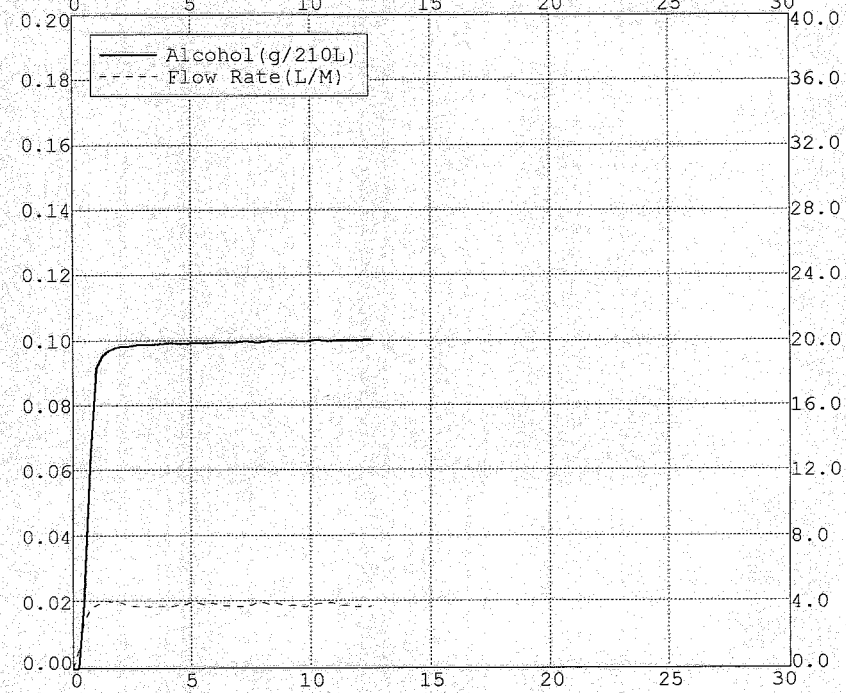

SOLUTION CHANGE

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

Date: 01/05/2020

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:52
INTERNAL STANDARD	VERIFIED	03:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:53
BLANK TEST	0.00	03:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:54
BLANK TEST	0.00	03:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:55
BLANK TEST	0.00	03:56

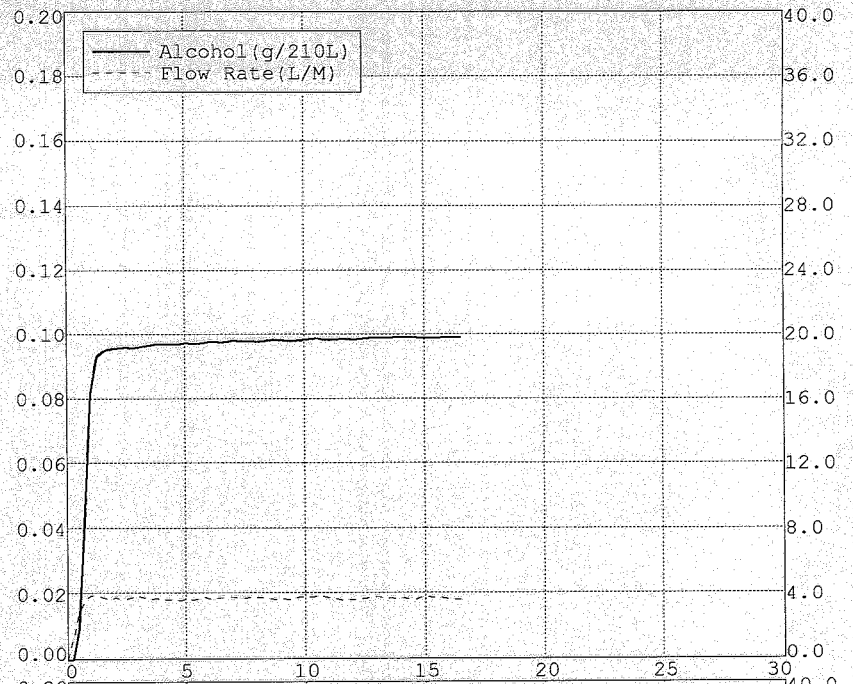

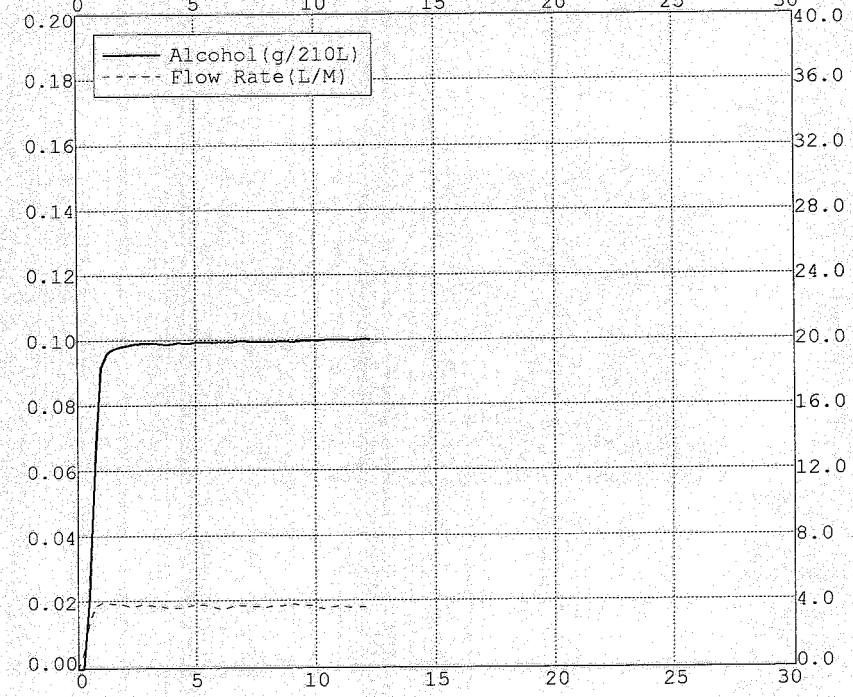

SUPERVISOR TEST

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

Date: 12/21/2019

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:11
INTERNAL STANDARD	VERIFIED	03:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:11
BLANK TEST	0.00	03:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:12
BLANK TEST	0.00	03:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:13
BLANK TEST	0.00	03:14

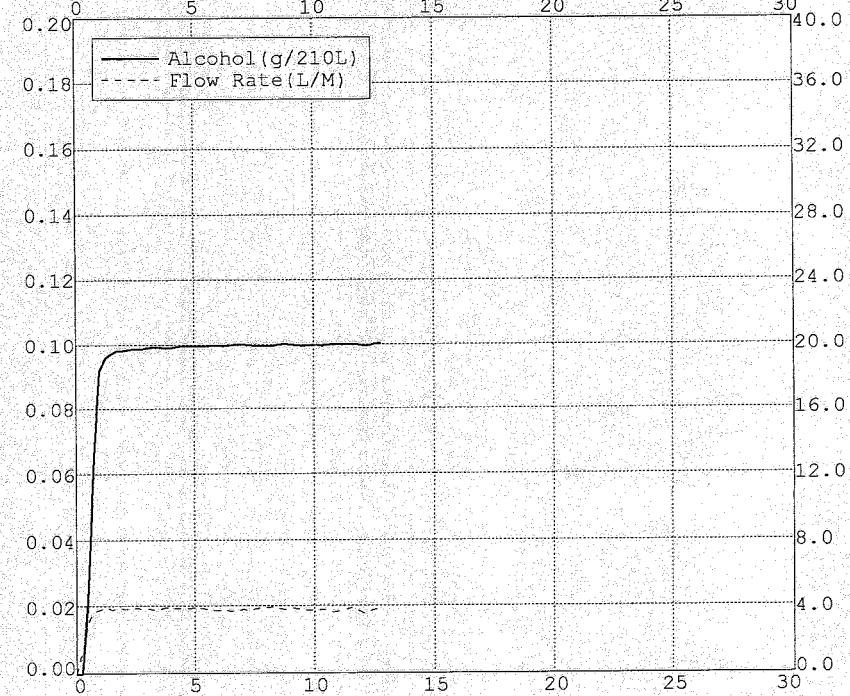

SUPERVISOR TEST

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

Date: 12/15/2019

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:13
INTERNAL STANDARD	VERIFIED	03:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:13
BLANK TEST	0.00	03:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:14
BLANK TEST	0.00	03:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:15
BLANK TEST	0.00	03:16

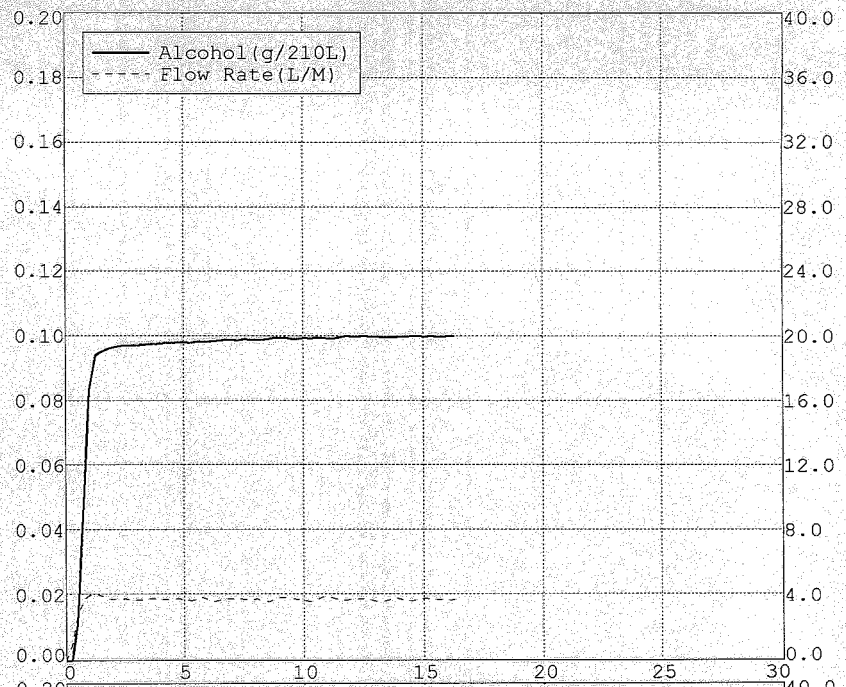

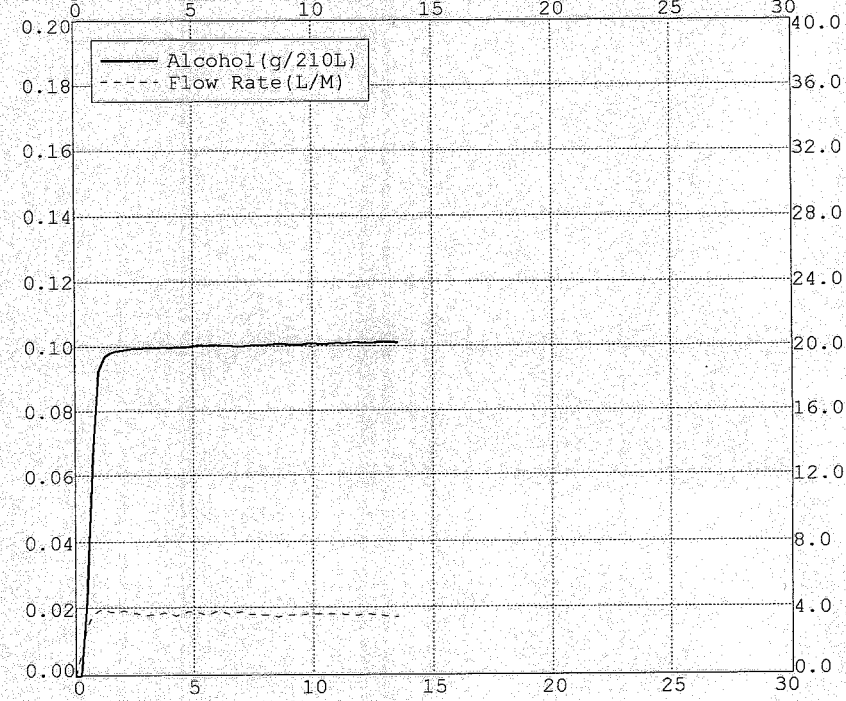

SOLUTION CHANGE

GRANVILLE VILLAGE
POLICE DEPT
DATAMASTER dmt: 113306

Date: 12/07/2019

OPERATOR NAME:
RYAN S PEDONE
Permit #: 35878
Operator Agency/Dept: GRANVILLE VILLAGE PD
Reference Standard #: 19250

Nominal = 0.10 g/210L
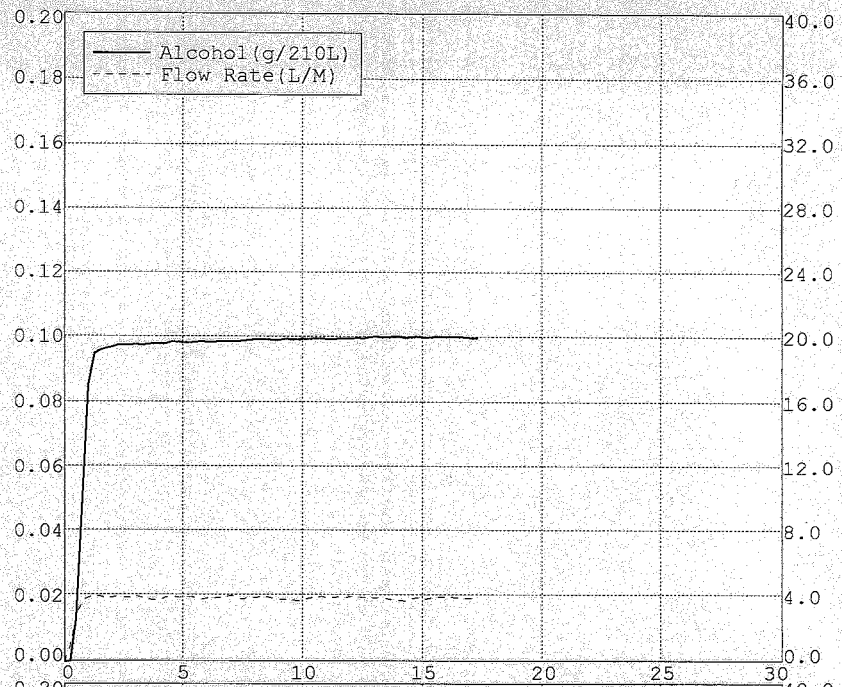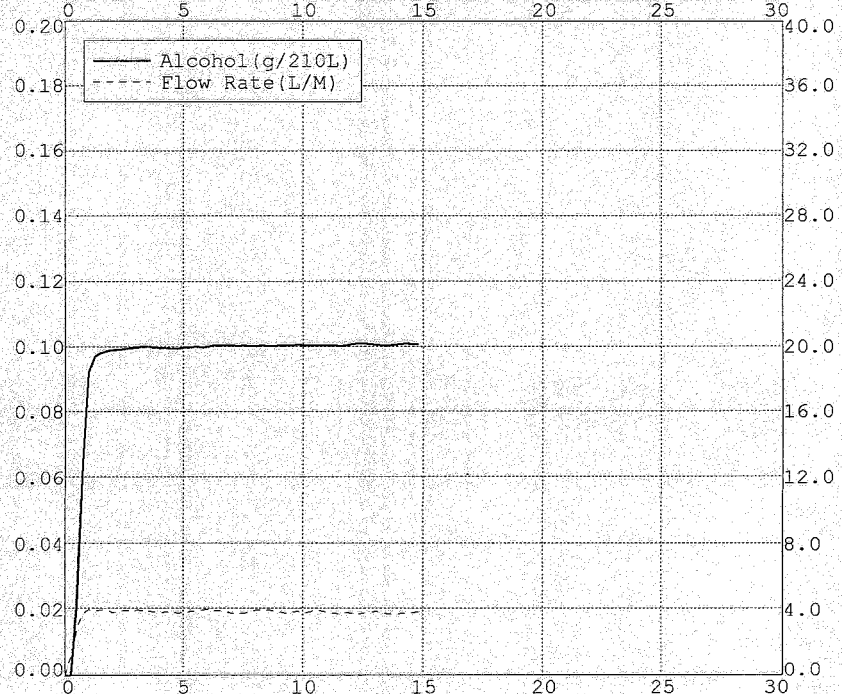
BLANK TEST	0.00	22:37
INTERNAL STANDARD	VERIFIED	22:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:38
BLANK TEST	0.00	22:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:39
BLANK TEST	0.00	22:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:40
BLANK TEST	0.00	22:41