

GPD

01-20-2020

1. Weekly Test for DMT

2. Jan. 2020      DMT      Cal  
    July 2019

SUPERVISOR TEST



GRANVILLE VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 113306

ate: 01/19/2020

OPERATOR NAME:  
RYAN S PEDONE  
Permit #: 35878  
Operator Agency/Dept: GRANVILLE VILLAGE PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:52
INTERNAL STANDARD	VERIFIED	21:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:52
BLANK TEST	0.00	21:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:54
BLANK TEST	0.00	21:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:55
BLANK TEST	0.00	21:55

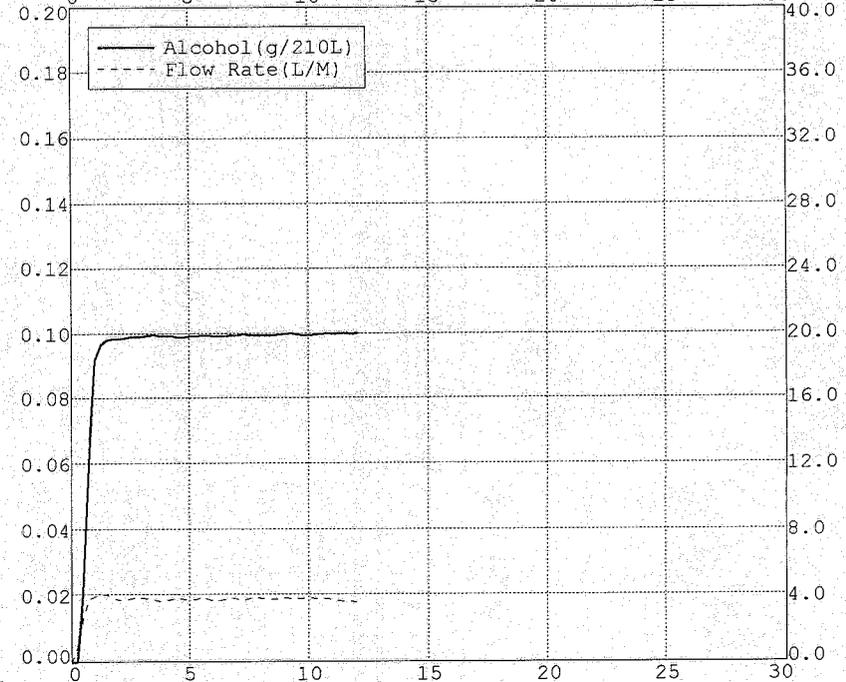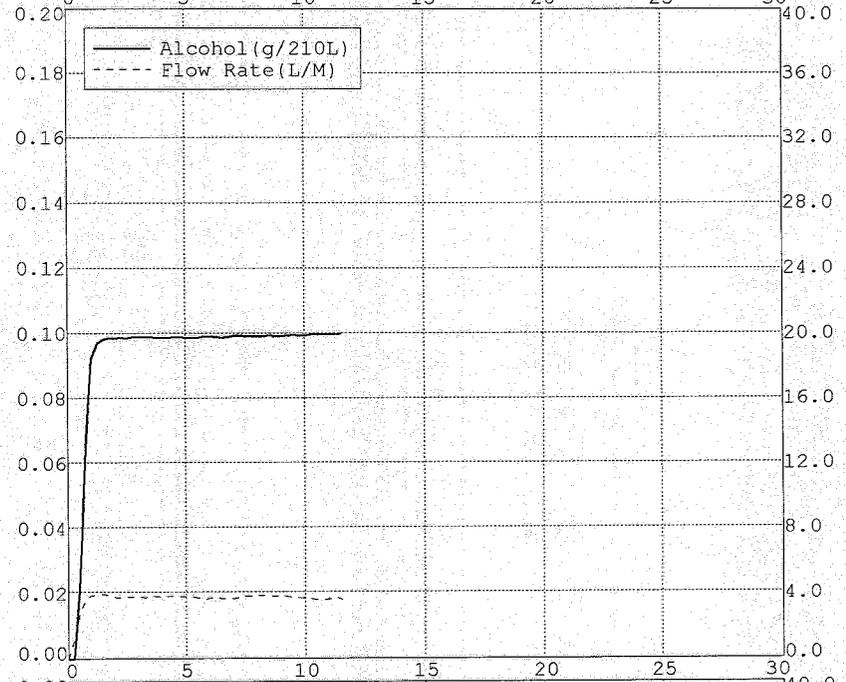



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS. DATAMASTER DMT breath test instrument, serial number 113306, performed on January 08, 2020 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

Digitally signed under ESRA  
by Joshua Vinehout  
on 1/10/2020 2:15 PM

**Joshua Vinehout**  
**Supervisor of Public Safety Programs**  
**Office of Public Safety**

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Granville Village Police Department  
Manufacturer: NAT'L PATENT ANALYTICAL SYS      Model: DATAMASTER DMT  
Serial Number: 113306  
Date: January 08, 2020


Reference Solution Lot Number: 19250  
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.01 degrees centigrade
2	0.100 %	34.01 degrees centigrade
3	0.100 %	34.01 degrees centigrade
4	0.100 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 113306, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
ESRA by Jonathan Mascolo  
on 1/8/2020 1:36 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 45339

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 1/10/2020 11:27 AM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Granville Village Police Department  
**Manufacturer:** NAT'L PATENT ANALYTICAL SYS  
**Model:** DATAMASTER DMT  
**Serial Number:** 113306  
**Date:** January 08, 2020

1. General Appearance and condition of this device \_\_\_\_\_: N/A


2. Check controls and indicators \_\_\_\_\_: OK

3. Check breath flow system \_\_\_\_\_: OK

4. Check printer operation \_\_\_\_\_: N/A

5. System cycles through all modes \_\_\_\_\_: OK

6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**

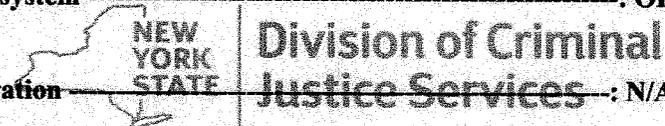

Performed by:

Digitally signed under  
ESRA by Jonathan Mascolo  
on 1/8/2020 1:36 PM

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 45339**

Reviewed by:

Digitally signed under  
ESRA by Frank Sgarlata  
on 1/10/2020 11:27 AM

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

Control Test Record

Simulator Information

Serial Number: 113306

Lot: 19250

Nominal: 0.100

Test Date: 01/05/2020 03:51:44

Test Results

Location: 03

Alcohol 1: 0.09

34.01

GRANVILLE POLICE DEPT.

Alcohol 2: 0.10

34.01

Supervisor Information

Alcohol 3: 0.10

34.01

First Name: Ryan S


Solution Change:

Last Name: Pedone

Permit: 35878

Agency: GRANVILLE VILLAGE PD

Plot 1 of 3 <=>

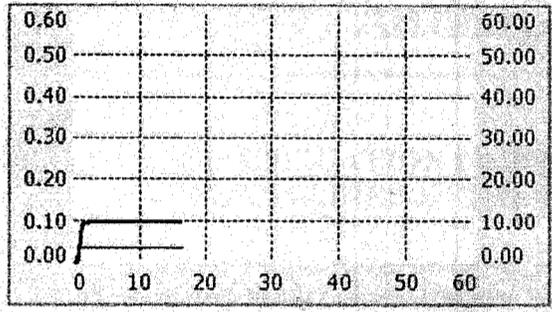

Status

Status Code:

Date Time:

Message:

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Granville Village Police Department  
 Manufacturer: NAT'L PATENT ANALYTICAL SYS      Model: DATAMASTER DMT  
 Date: July 19, 2019      Serial Number: 113306

Reference Solution Lot Number: 18371  
 Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.097 %	34.01 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.098 %	34.01 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number: 19101  
 Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.081 %	34.01 degrees centigrade
2	0.081 %	34.01 degrees centigrade
3	0.082 %	34.01 degrees centigrade
4	0.081 %	34.01 degrees centigrade


Reference Solution Lot Number: 18280  
 Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.182 %	34.01 degrees centigrade
2	0.182 %	34.01 degrees centigrade
3	0.181 %	34.01 degrees centigrade
4	0.183 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 113306, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
 ESRA by Martin Schilling  
 on 7/19/2019 10:56 AM

**Martin Schilling**  
 Highway Safety Equipment Technician  
 Breath Analysis Operator Permit # 45926

Reviewed by:




Digitally signed under  
 ESRA by Frank Sgarlata  
 on 7/22/2019 9:46 AM

**Frank Sgarlata**  
 Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Granville Village Police Department**  
**Manufacturer: NAT'L PATENT ANALYTICAL SYS**  
**Model: DATAMASTER DMT**  
**Serial Number: 113306**  
**Date: July 19, 2019**

- 1. General Appearance and condition of this device \_\_\_\_\_: OK
  
- 2. Check controls and indicators \_\_\_\_\_: OK
  
- 3. Check breath flow system \_\_\_\_\_: OK
  
- 4. Check printer operation \_\_\_\_\_: OK
  
- 5. System cycles through all modes \_\_\_\_\_: OK

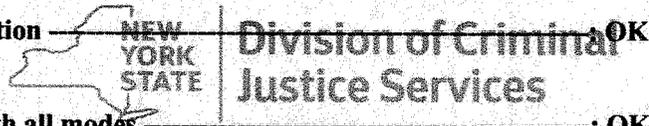

**6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION**

Performed by:

A handwritten signature in black ink, appearing to read "Martin Schilling".

Digitally signed under  
ESRA by Martin Schilling  
on 7/19/2019 10:56 AM

---

**Martin Schilling**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 45926**

Reviewed by:

A handwritten signature in black ink, appearing to read "Frank Sgarlata".

Digitally signed under  
ESRA by Frank Sgarlata  
on 7/22/2019 9:46 AM

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

TECHNICIAN TEST

GRANVILLE VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 113306





Date: 07/19/2019

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: GRANVILLE VILLAGE PD  
 Reference Standard #: 18371

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:04
INTERNAL STANDARD	VERIFIED	10:04
Xq = 0.094 (0.83%)		
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.097	10:04
X[1] = 0.0977 (-0.0014) (-0.0014)		
BLANK TEST	0.000	10:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	10:06
X[1] = 0.0990 (0.0003) (-0.0001)		
BLANK TEST	0.000	10:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	10:07
X[1] = 0.0987 (0.0001) (0.0006)		
BLANK TEST	0.000	10:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	10:08
X[1] = 0.0991 (-0.0001) (-0.0002)		
BLANK TEST	0.000	10:09

Average = 0.0982  
 Std Dev = 0.0010

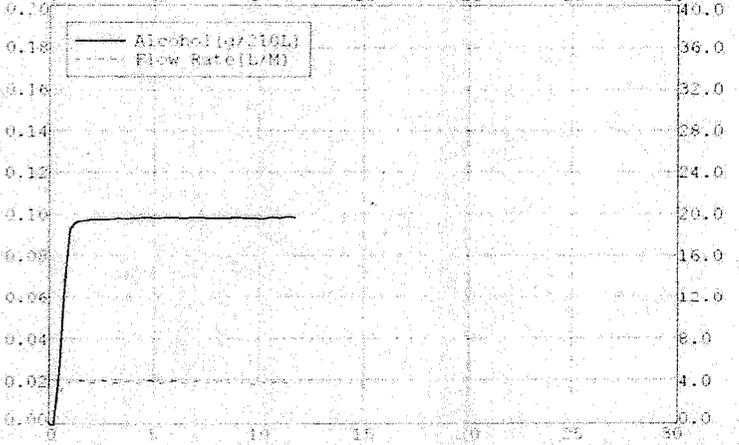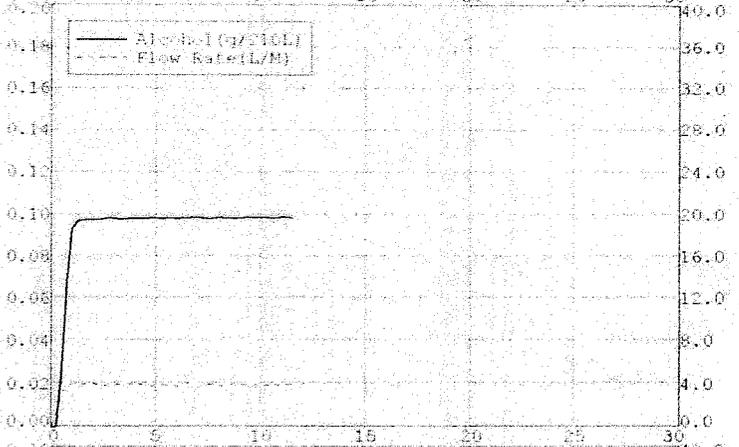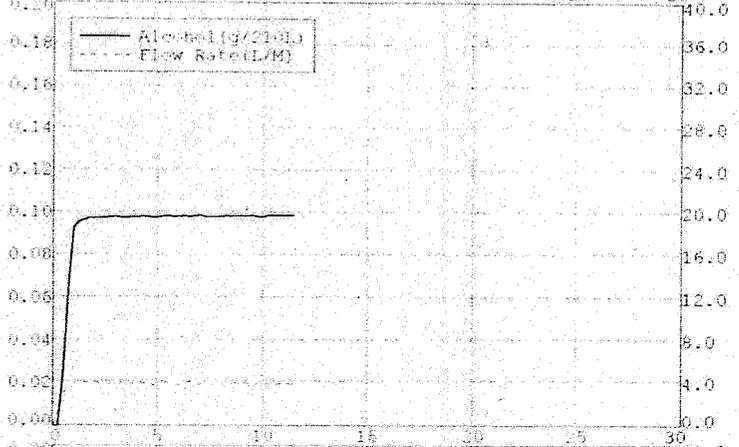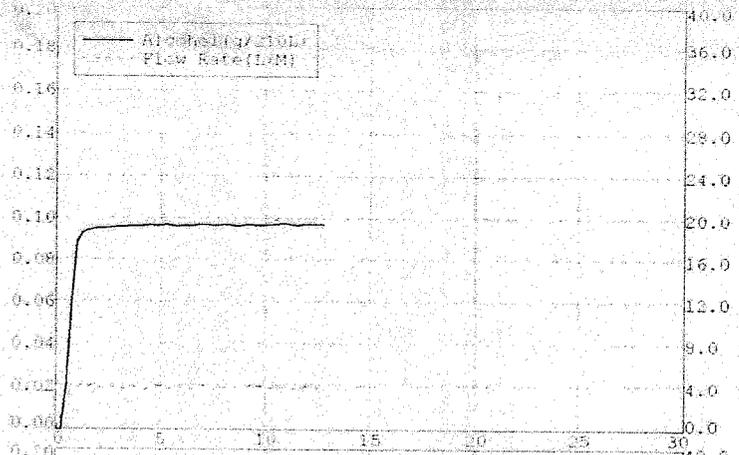

TECHNICIAN TEST

GRANVILLE VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 113306





Date: 07/19/2019

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: GRANVILLE VILLAGE PD  
 Reference Standard #: 19101

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:11
INTERNAL STANDARD	VERIFIED	10:11
Xq = 0.096 (0.83%)		
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	10:11
X[1] = 0.0813 (0.0004) (0.0001)		
BLANK TEST	0.000	10:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	10:12
X[1] = 0.0812 (-0.0006) (0.0008)		
BLANK TEST	0.000	10:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.082	10:13
X[1] = 0.0821 (0.0001) (0.0008)		
BLANK TEST	0.000	10:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	10:14
X[1] = 0.0816 (-0.0008) (0.0006)		
BLANK TEST	0.000	10:15

Average = 0.0812  
 Std Dev = 0.0005

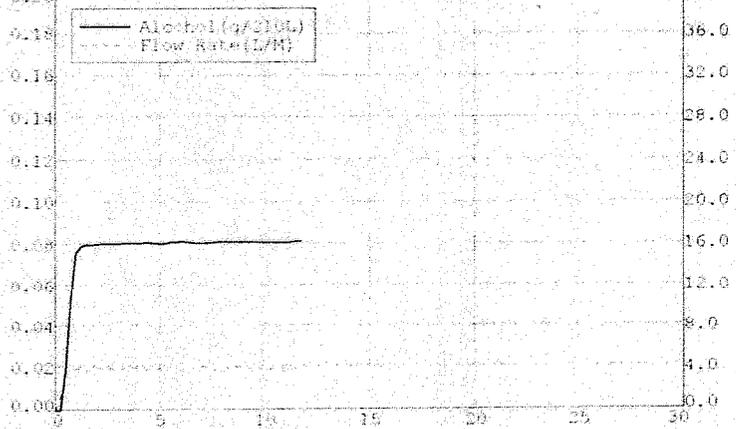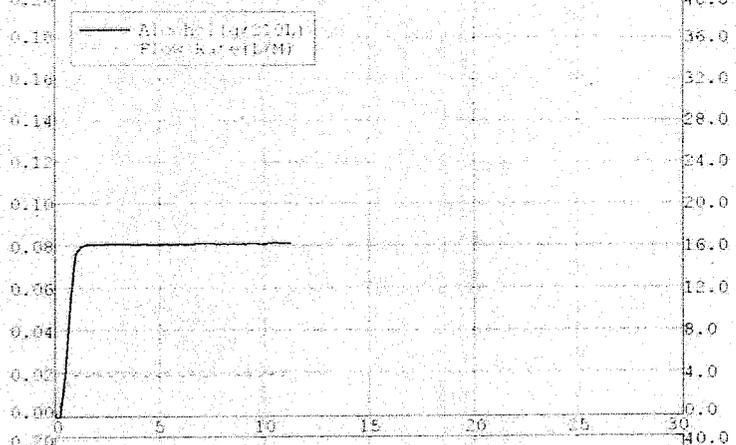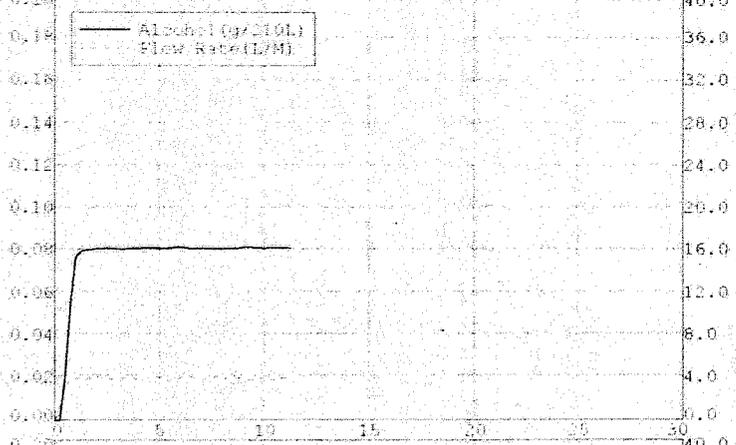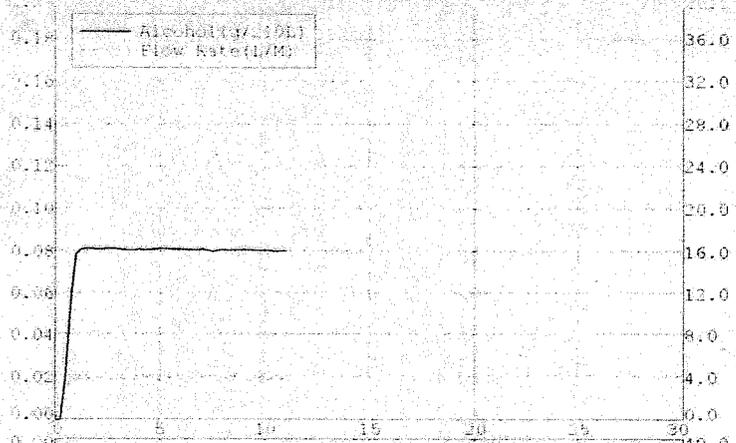

TECHNICIAN TEST

GRANVILLE VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 113306


Date: 07/19/2019

OPERATOR NAME:  
 MARTIN J SCHILLING  
 Permit #: 45926  
 Operator Agency/Dept: GRANVILLE VILLAGE PD  
 Reference Standard #: 18280

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:17
INTERNAL STANDARD	VERIFIED	10:17
Xq = 0.096 (1.01%)		
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.182	10:18
X[1] = 0.1825 (0.0007) (0.0014)		
BLANK TEST	0.000	10:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.182	10:19
X[1] = 0.1826 (0.0006) (0.0000)		
BLANK TEST	0.000	10:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.181	10:20
X[1] = 0.1817 (-0.0005) (-0.0002)		
BLANK TEST	0.000	10:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	10:21
X[1] = 0.1830 (0.0003) (0.0004)		
BLANK TEST	0.000	10:22

Average = 0.1820  
 Std Dev = 0.0008

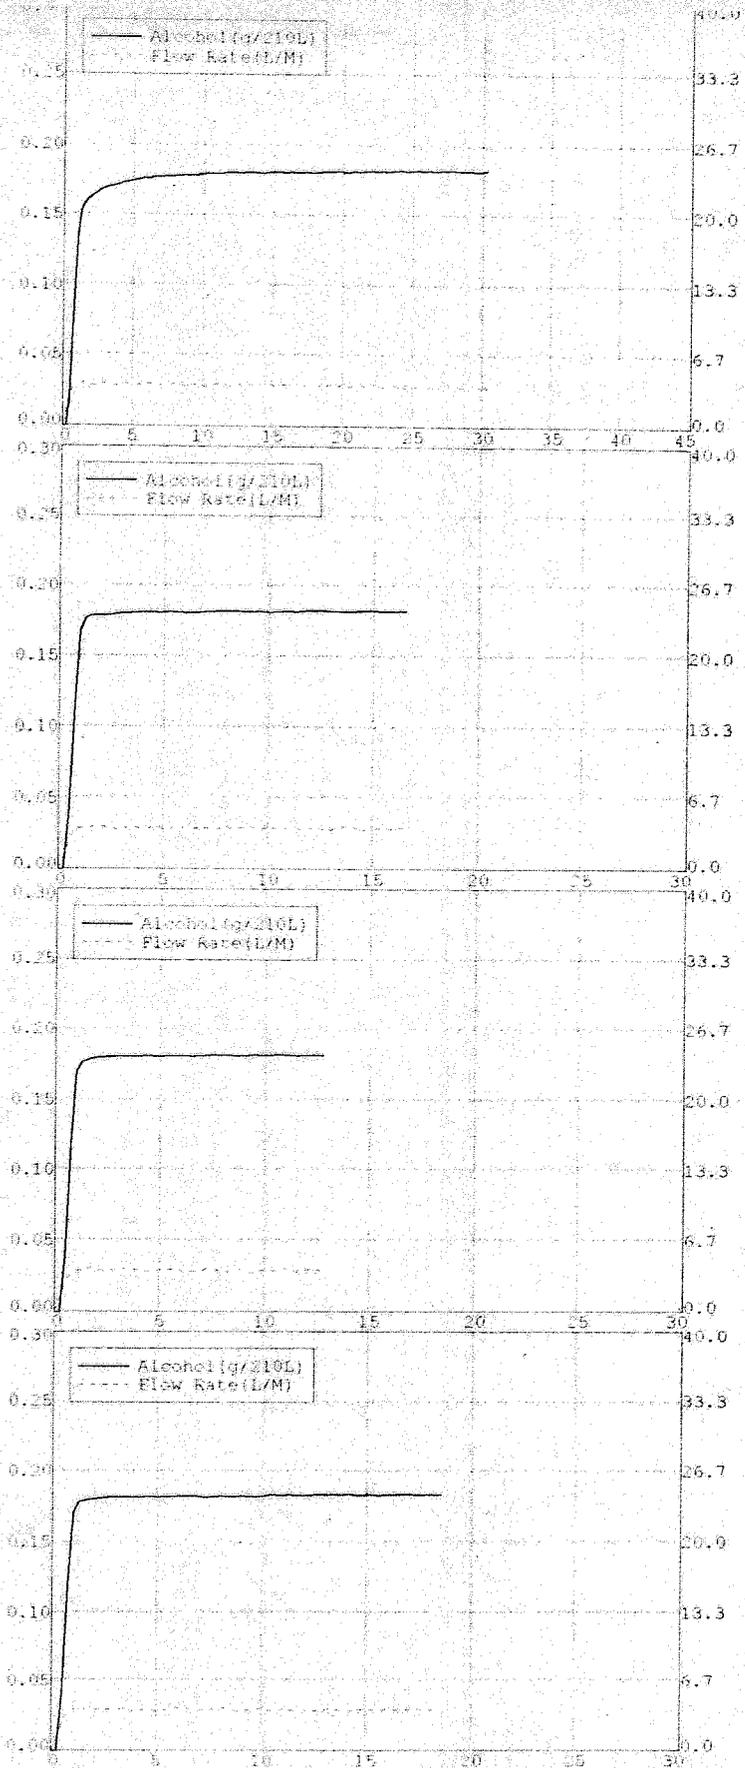

New York State Division of Criminal Justice Services  
**SERVICE AUTHORIZATION FORM**

*MJS*  
*7/19/19*

*GPD DTT*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE.

**SECTION I - AGENCY INFORMATION**

Name of Agency Granville Police Department		Today's Date 7/19/2019
Address 51 Quaker Street		City, State, ZIP Granville, N.Y. 12832
Contact Person Chief Ernie Bassette		Contact Telephone 518-642-2946
Contact Telephone 518-642-1414	Contact Facsimile 518-642-2946	Contact Email granvillepd101@hotmail.com

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer Datamaster		Model Number DMT
Instrument Serial Number 113306	Antenna Serial Number (if applicable)	
Date of Malfunction	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction BiYearly Certification		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units. Repco Simulator Serial Number 0397 Over heats at times and shuts down Keyboard Hoses		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein.		
Signature 		Date 7/19/2019

**DCJS USE ONLY**

<p>2.00-5  <i>Inspected instrument. Checked setup voltage point and remote operation. Performed calibration/adjustment procedure. Ran subject, testing and diagnostic tests. Verified calibration.</i></p>
--