

SUPERVISOR TEST

CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 01/27/2020

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 19250

Nominal = 0.10 g/210L




BLANK TEST	0.00	07:05	
INTERNAL STANDARD	VERIFIED	07:05	
REFERENCE STANDARD TEMP	34.00c		
REFERENCE STANDARD	0.09	07:06	
BLANK TEST	0.00	07:06	
REFERENCE STANDARD TEMP	34.00c		
REFERENCE STANDARD	0.09	07:07	
BLANK TEST	0.00	07:08	
REFERENCE STANDARD TEMP	34.00c		
REFERENCE STANDARD	0.09	07:08	
BLANK TEST	dmt: 126706	0.00	07:09

Date: 01/27/2020

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:05
INTERNAL STANDARD	VERIFIED	07:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:06
BLANK TEST	0.00	07:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:07
BLANK TEST	0.00	07:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:08
BLANK TEST	0.00	07:09

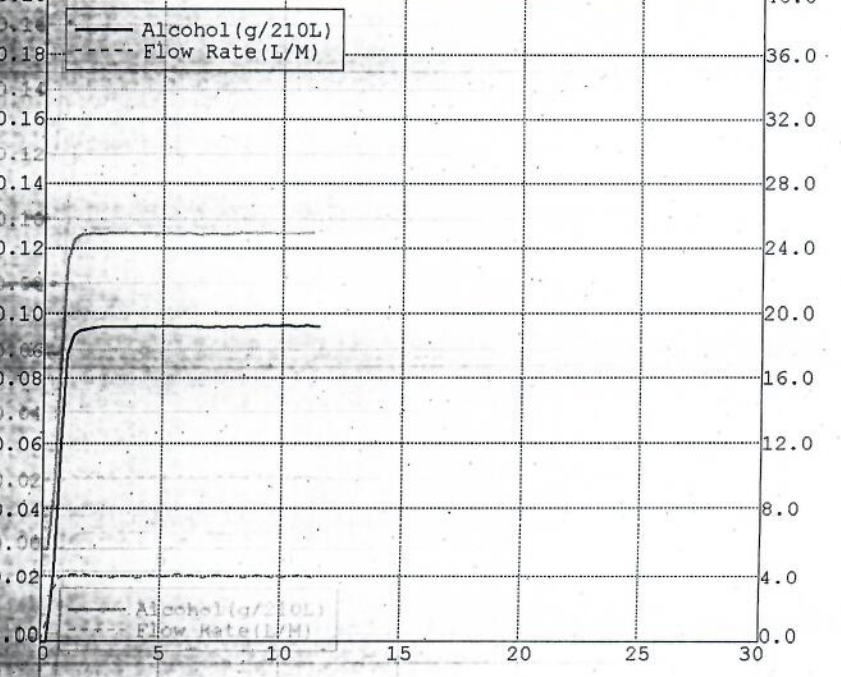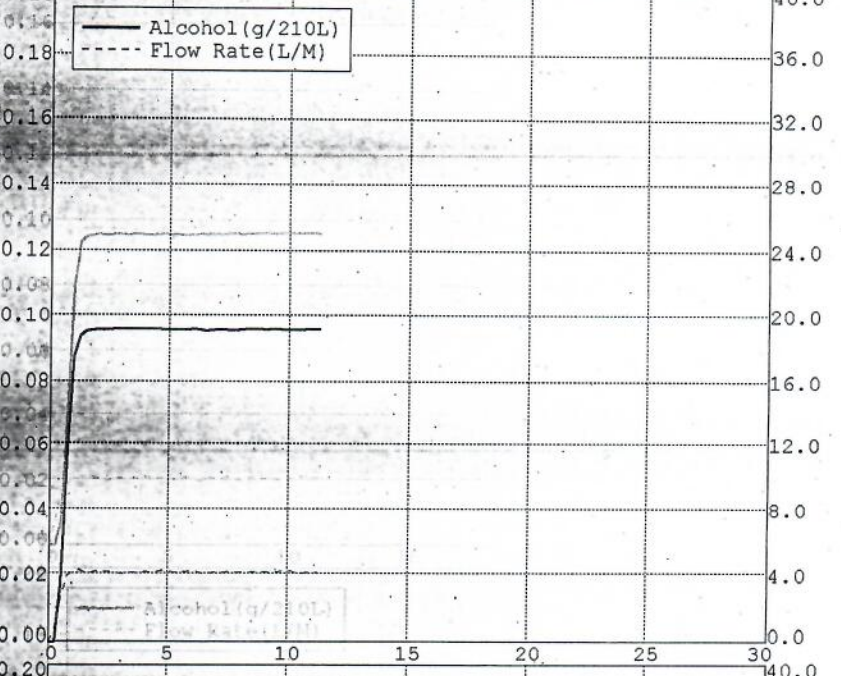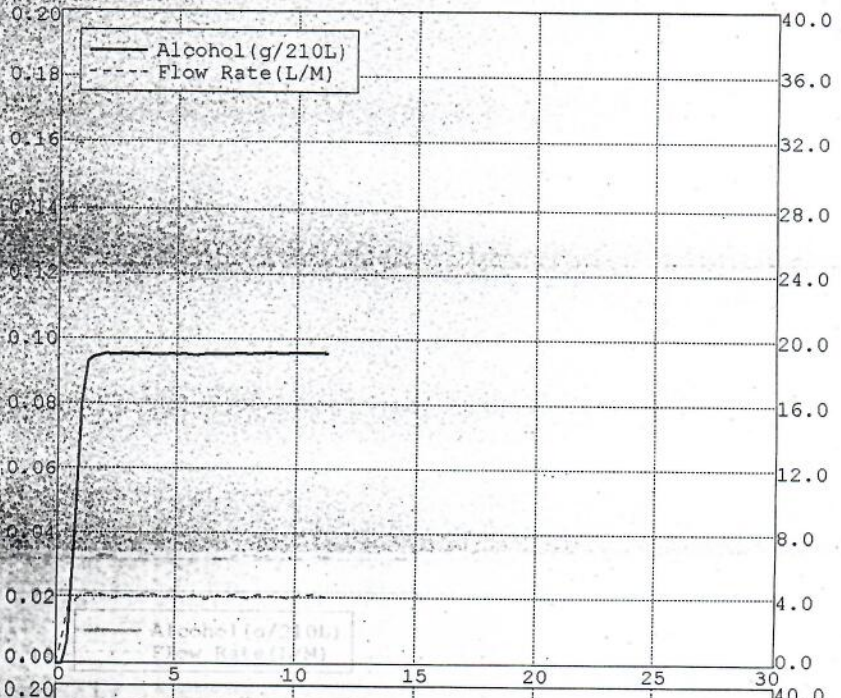

SUPERVISOR TEST

CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 01/20/2020

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:08
INTERNAL STANDARD	VERIFIED	07:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:08
BLANK TEST	0.00	07:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:09
BLANK TEST	0.00	07:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:11
BLANK TEST dmt: 126706	0.00	07:11

Date: 01/20/2020

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:08
INTERNAL STANDARD	VERIFIED	07:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:08
BLANK TEST	0.00	07:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:09
BLANK TEST	0.00	07:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:11
BLANK TEST	0.00	07:11

