



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 126706, performed on January 13, 2020 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 1/15/2020 2:25 PM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cambridge Village Police Department

Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT

Date: January 13, 2020

Serial Number: 126706

Reference Solution Lot Number: 19281

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	33.99 degrees centigrade
2	0.099 %	33.99 degrees centigrade
3	0.099 %	34.00 degrees centigrade
4	0.099 %	33.99 degrees centigrade

Reference Solution Lot Number: 19101

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.081 %	33.99 degrees centigrade
2	0.080 %	34.00 degrees centigrade
3	0.080 %	34.00 degrees centigrade
4	0.081 %	33.99 degrees centigrade

Reference Solution Lot Number: 19210

Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.184 %	33.99 degrees centigrade
2	0.185 %	33.99 degrees centigrade
3	0.184 %	34.00 degrees centigrade
4	0.185 %	33.99 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 126706, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Joseph Iavarone
on 1/13/2020 3:41 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 1/15/2020 1:03 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cambridge Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 126706
Date: January 13, 2020

1. General Appearance and condition of this device -----: OK

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: OK

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.



Performed by:

Joseph Iavarone

Digitally signed under
ESRA by Joseph Iavarone
on 1/13/2020 3:41 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:

Frank Sgarlata

Digitally signed under
ESRA by Frank Sgarlata
on 1/15/2020 1:03 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

CAMBRIDGE VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 126706





Date: 01/13/2020

OPERATOR NAME:
 JOSEPH A IAVARONE
 Permit #: 44106
 Operator Agency/Dept: CAMBRIDGE VILL. PD
 Reference Standard #: 19101

Nominal = 0.080 g/210L

BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.081	13:28
BLANK TEST	0.000	13:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	13:29
BLANK TEST	0.000	13:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	13:30
BLANK TEST	0.000	13:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.081	13:31
BLANK TEST	0.000	13:32

Average = 0.0805
 Std Dev = 0.0006

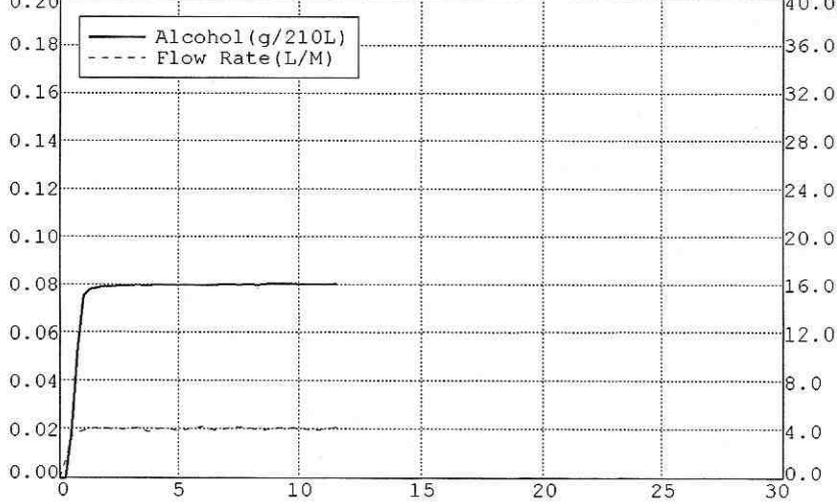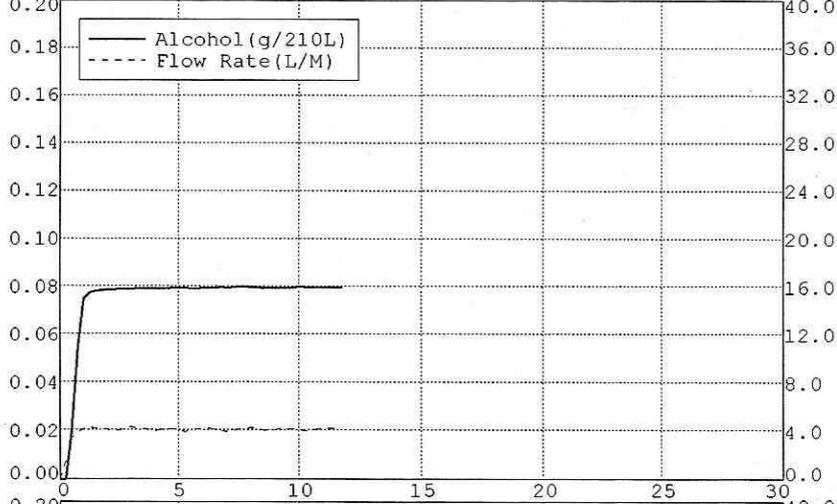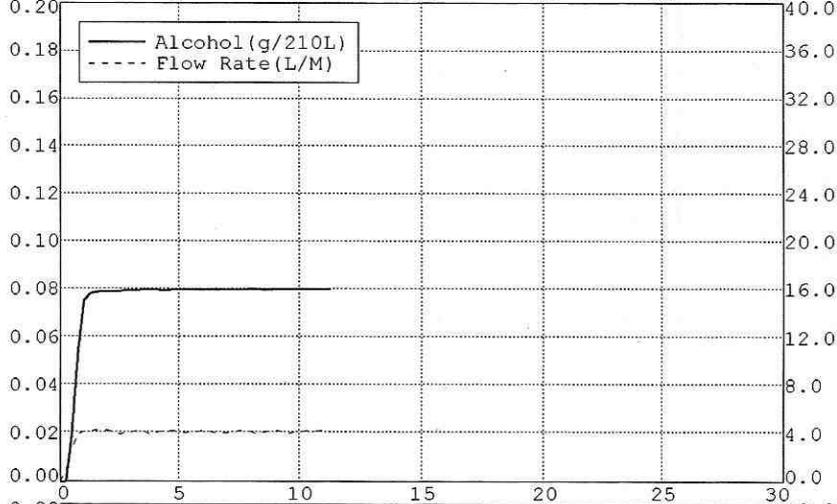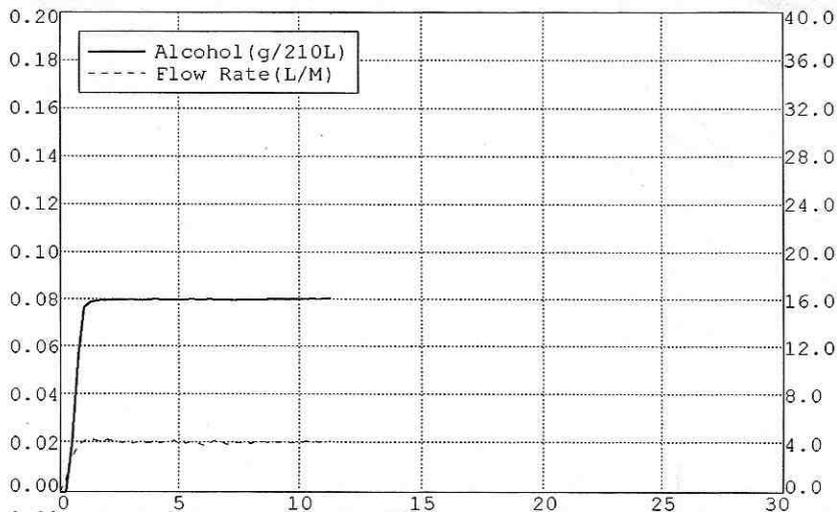

TECHNICIAN TEST

 CAMBRIDGE VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 126706





Date: 01/13/2020

OPERATOR NAME:
 JOSEPH A IAVARONE
 Permit #: 44106
 Operator Agency/Dept: CAMBRIDGE VILL. PD
 Reference Standard #: 19281

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.100	12:19
BLANK TEST	0.000	12:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.099	12:21
BLANK TEST	0.000	12:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.099	12:22
BLANK TEST	0.000	12:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.099	12:23
BLANK TEST	0.000	12:24

Average = 0.0992
 Std Dev = 0.0005

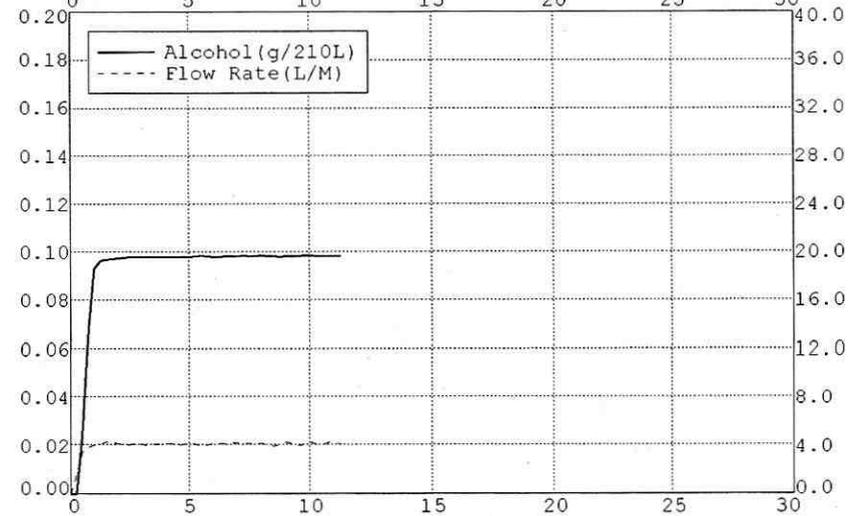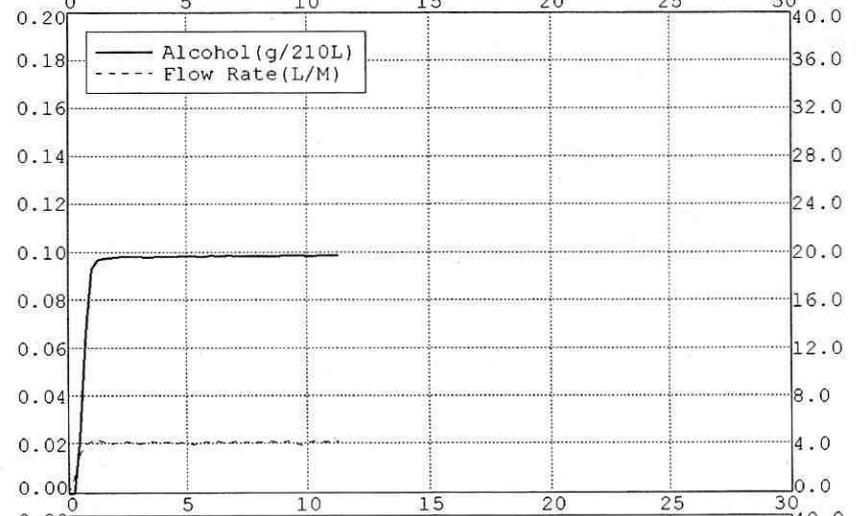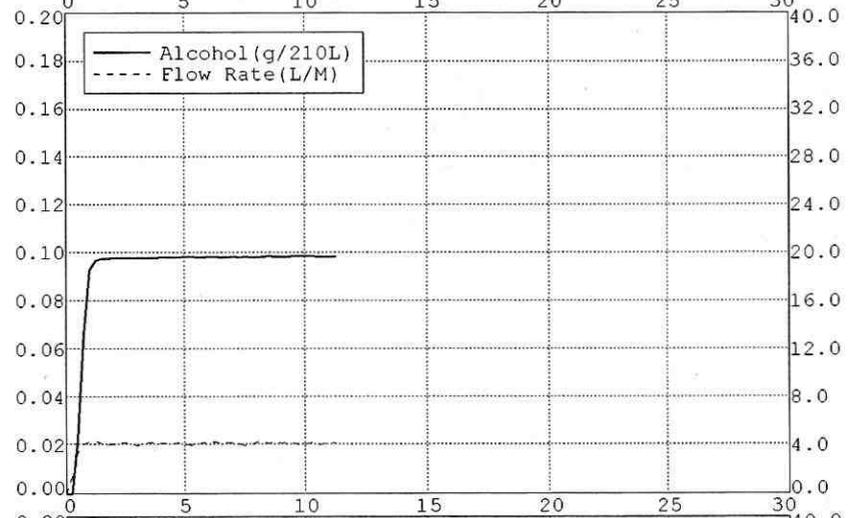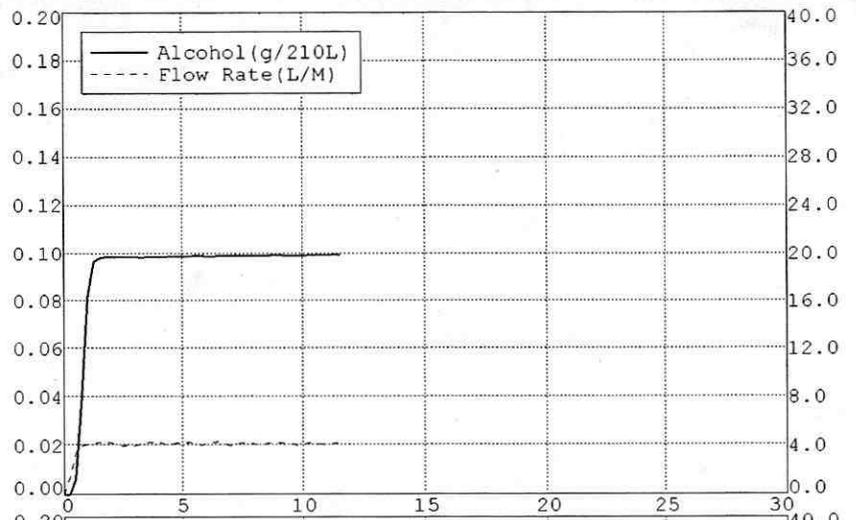

TECHNICIAN TEST

CAMBRIDGE VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 126706





Date: 01/13/2020

OPERATOR NAME:
 JOSEPH A IAVARONE
 Permit #: 44106
 Operator Agency/Dept: CAMBRIDGE VILL. PD
 Reference Standard #: 19210

Nominal = 0.180 g/210L

BLANK TEST	0.000	13:47
INTERNAL STANDARD	VERIFIED	13:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.184	13:48
BLANK TEST	0.000	13:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.185	13:49
BLANK TEST	0.000	13:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.184	13:50
BLANK TEST	0.000	13:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.185	13:51
BLANK TEST	0.000	13:52

Average = 0.1845
 Std Dev = 0.0006

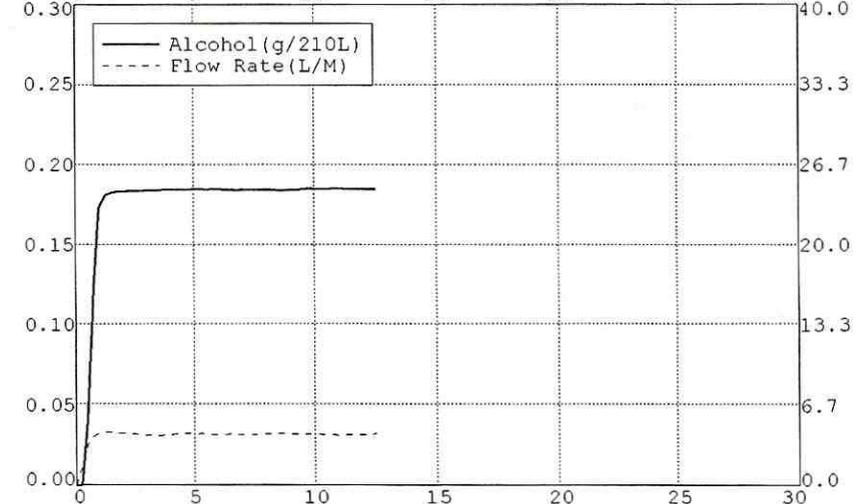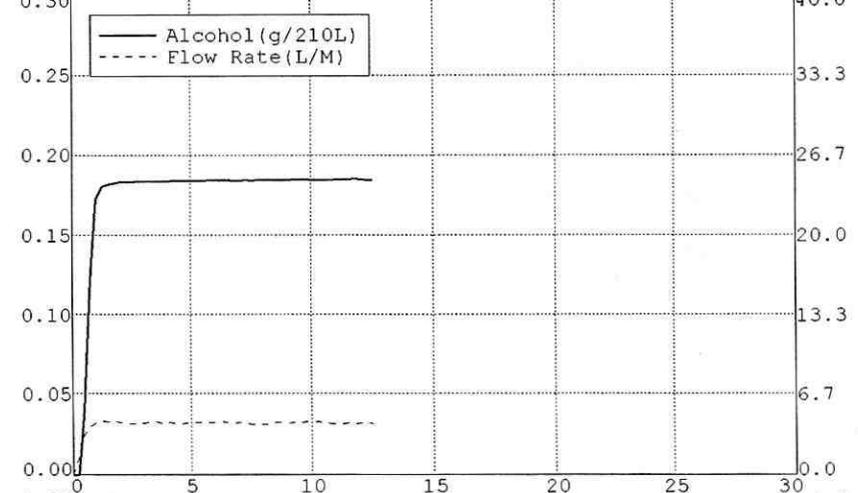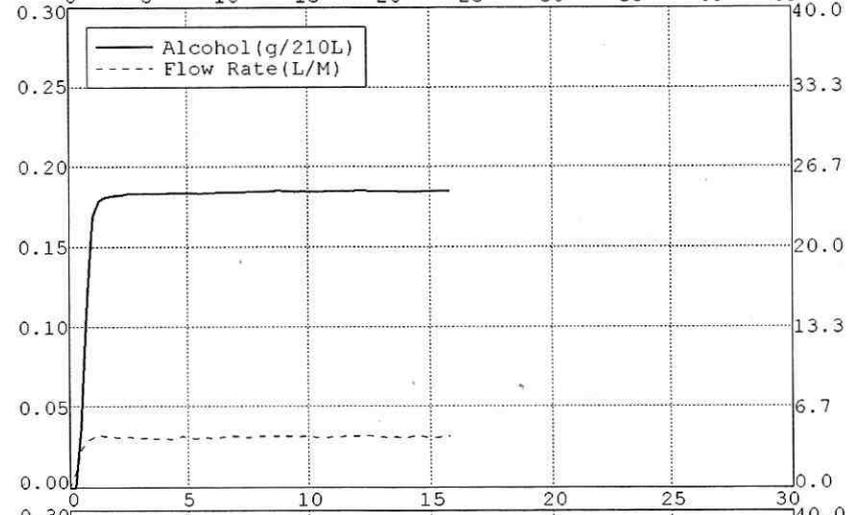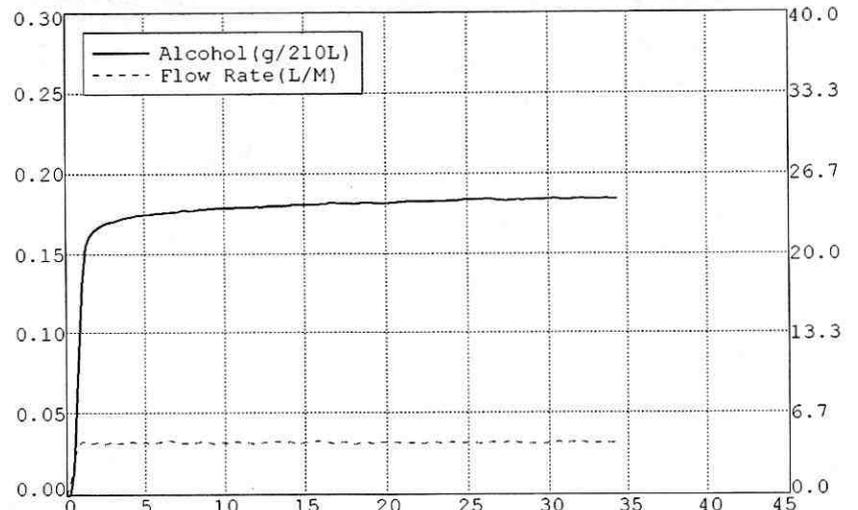

New York State Division of Criminal Justice Services
SERVICE AUTHORIZATION FORM

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE.

SECTION I - AGENCY INFORMATION

Name of Agency Cambridge Greenwich PD		Today's Date 1-13-2020
Address 56 North Park St		City, State, ZIP Cambridge, NY, 12816
Contact Person Officer Davis-Flynn		Contact Telephone 518-209-7141
Contact Telephone	Contact Facsimile	Contact Email

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer DATA MASTER DMT		Model Number
Instrument Serial Number 126706	Antenna Serial Number (if applicable)	
Date of Malfunction	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units. DATA Master, Keyboard, SIM Tube, Breath Tube, Plug Power Cable		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein.		
Signature PT: [Signature]		Date 01-13-20

DCJS USE ONLY

Inspected instrument, checked setup voltages, print and remote operation, performed calibration/adjustment procedure, ran subject, technician and diagnostic tests, verified calibration.
