SUPERVISOR TEST

FORT EDWARD
VILLAGE POLICE DEPT.
DATAMASTER dmt: 115708

Date: 07/26/2021

OPERATOR NAME:
SGT DEAN E WATKINS
Permit #: 39523
Operator Agency/Dept: FORT EDWARD VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L
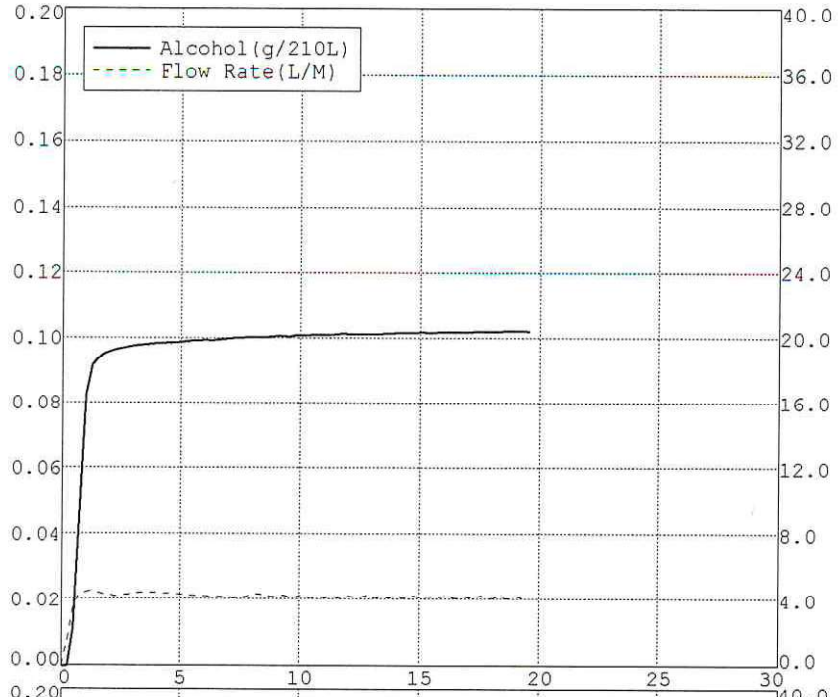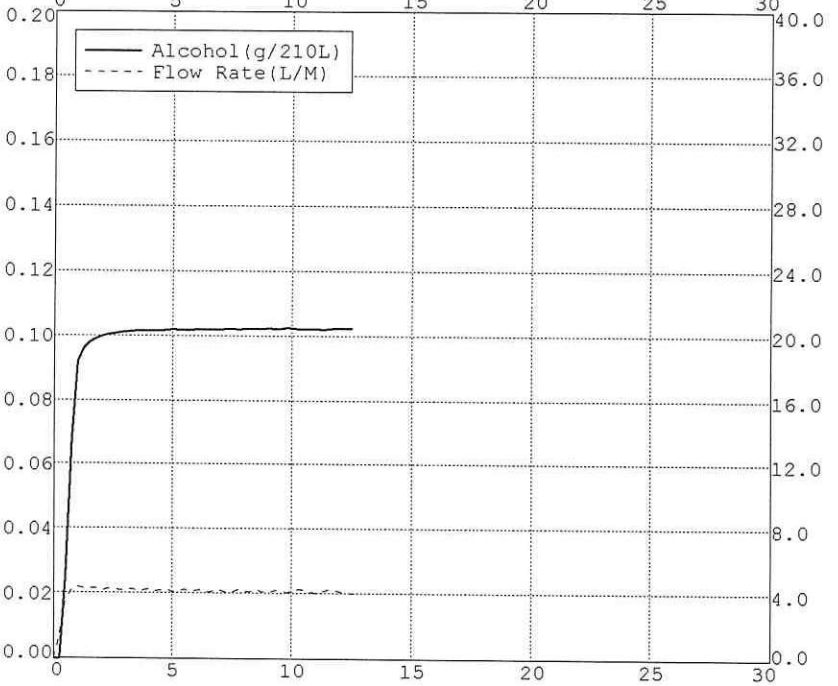
BLANK TEST	0.00	22:52
INTERNAL STANDARD	VERIFIED	22:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:53
BLANK TEST	0.00	22:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:54
BLANK TEST	0.00	22:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:55
BLANK TEST	0.00	22:56